

Scheme: Sperm-hyaluronan assay

Distribution: Q1/4 - 2021/2022

Lab name: LabMagister

Lab number: 971

Reviewed by:


Date:

Action taken:


I Dr Mikus Endre on behalf of LabMagister have read and agreed to the terms and conditions outlined by EQASRM.

Sample code	HB385	HB386	HB387	HB388
Description	Semen sample I	Semen sample II	Semen sample III	Semen sample IV
Number of returns	4	4	4	4
Responses for normal maturity/physiological function	Yes 4/4 No 0/4	Yes 4/4 No 0/4	Yes 4/4 No 0/4	Yes 4/4 No 0/4
Your result (% sperm bound to slide)	94.9	91.4	87.1	92.8
Does this indicate normal maturity/physiological function?	Yes	Yes	Yes	Yes
Comment	Acceptable	Acceptable	Acceptable	Acceptable
Overall statistic				
Mean	94.2	93.4	90.3	95.2
SD	0.9	1.9	3.0	1.6
Range	[93-95]	[91.4-96]	[87.1-94]	[92.8-96]
Your bias	0.7%	-2.1%	-3.5%	-2.5%
Points to note				


HB385




HB386

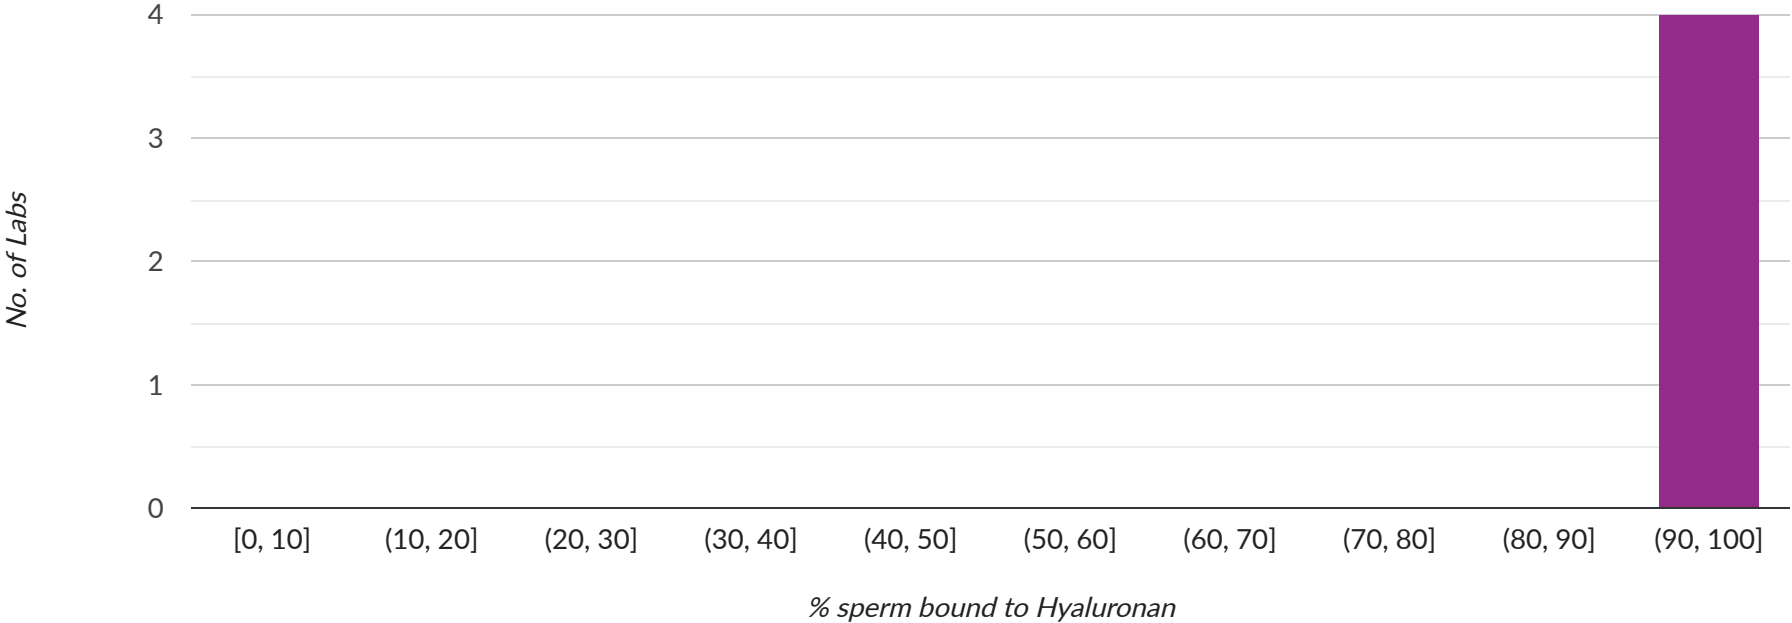


HB387



HB388



Bias



You can alter the date range of results by grabbing and sliding the ends of this section.

