

Scheme: Sperm-hyaluronan assay

Distribution: Q1/4 - 2023/2024

Lab name: LabMagister

Lab number: 971

Reviewed by:


Date:

Action taken:


I Dr Mikus Endre on behalf of LabMagister have read and agreed to the terms and conditions outlined by EQASRM.

Sample code	HB417	HB418	HB419	HB420
Description	Semen sample I	Semen sample II	Semen sample III	Semen sample IV
Number of returns	4	4	4	4
Responses for normal maturity/physiological function	Yes 3/4 No 1/4	Yes 4/4 No 0/4	Yes 4/4 No 0/4	Yes 3/4 No 1/4
Your result (% sperm bound to slide)	74	87	85	82
Does this indicate normal maturity/physiological function?	No	Yes	Yes	Yes
Comment	Acceptable	Acceptable	Acceptable	Acceptable
Overall statistic				
Mean	79.2	89.2	89	81.2
SD	5.7	2.1	3.7	2.9
Range	[74-86]	[87-91]	[85-94]	[79-85]
Your bias	-6.6%	-2.5%	-4.5%	1.0%
Points to note				


HB417

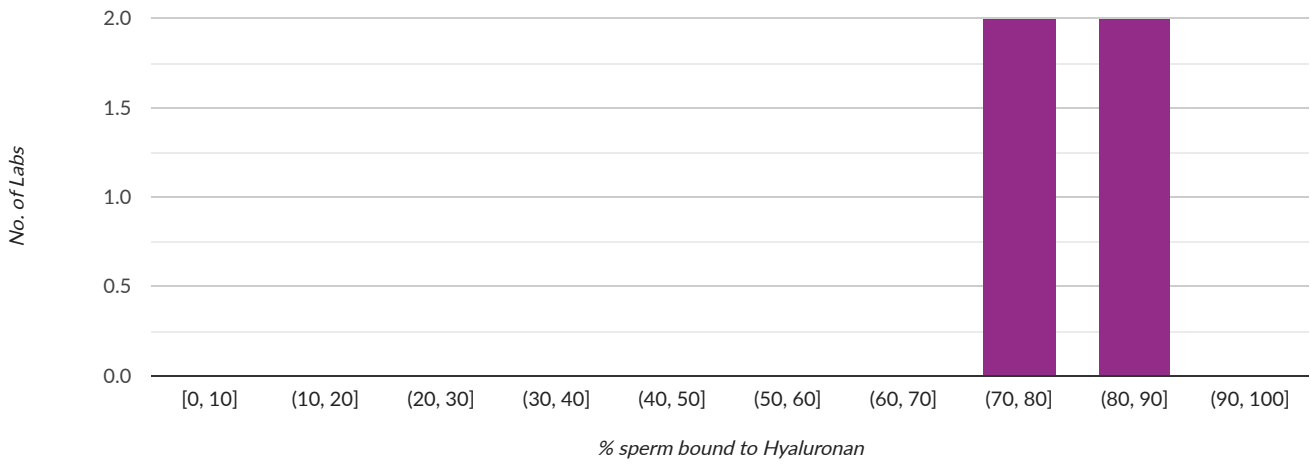


HB418

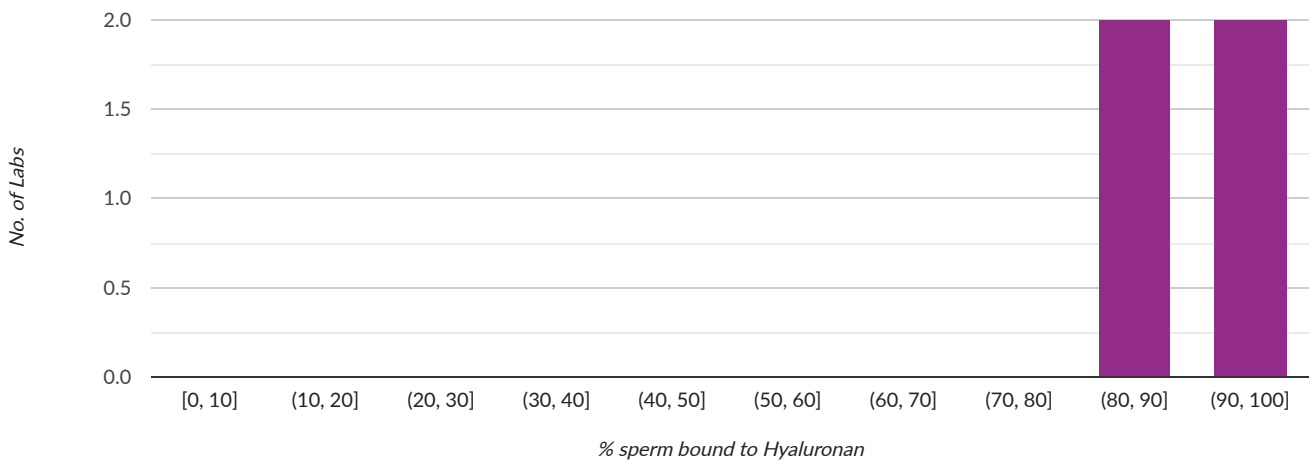


HB419

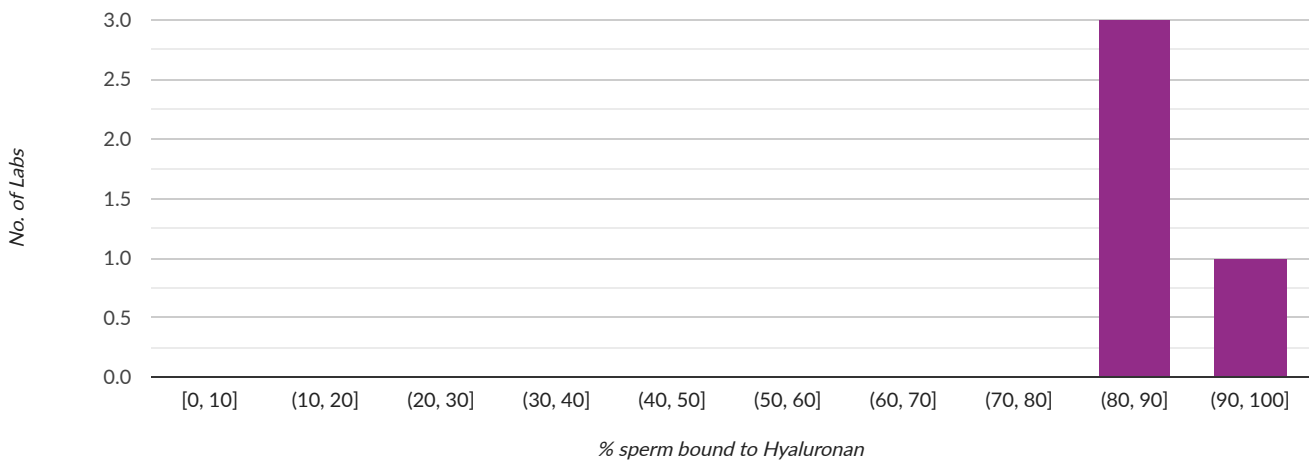

HB420

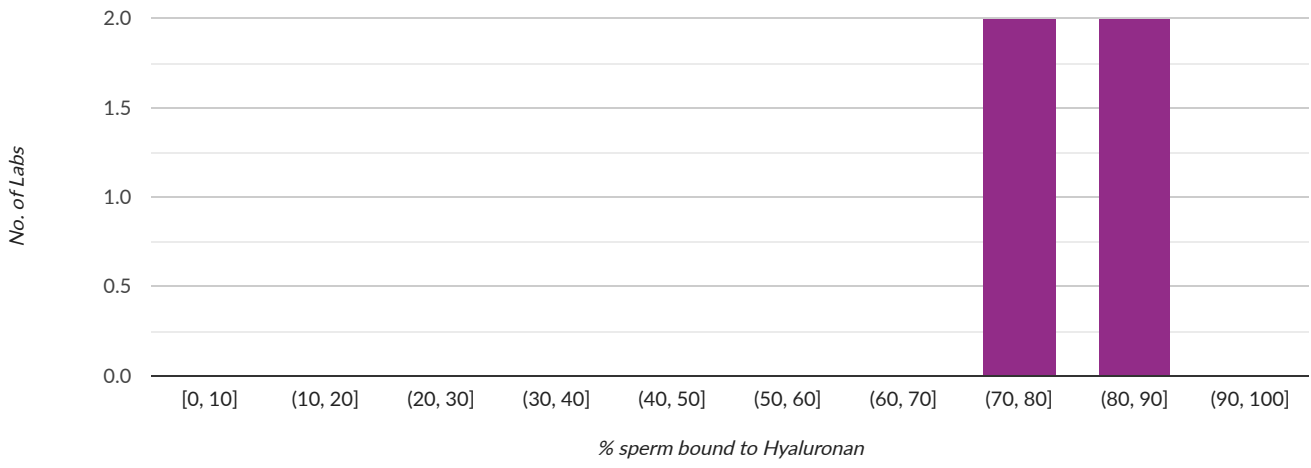

Bias

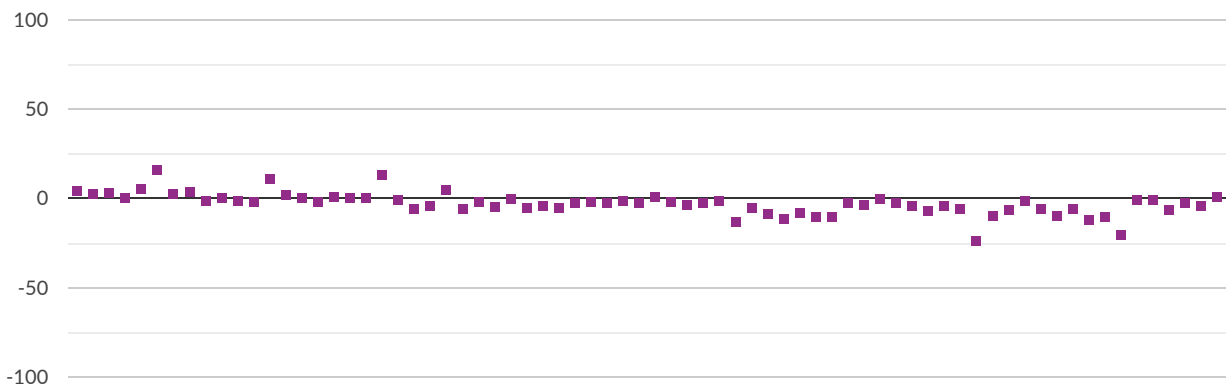

You can alter the date range of results by grabbing and sliding the ends of this section.

