

Scheme: Sperm-hyaluronan assay

Distribution: Q3/4 - 2023/2024

Lab name: LabMagister

Lab number: 971

Reviewed by:


Date:

Action taken:


I Dr Mikus Endre on behalf of LabMagister have read and agreed to the terms and conditions outlined by EQASRM.

Sample code	HB425	HB426	HB427	HB428
Description	Semen sample I	Semen sample II	Semen sample III	Semen sample IV
Number of returns	4	4	4	4
Responses for normal maturity/physiological function	Yes 4/4 No 0/4	Yes 3/4 No 1/4	Yes 4/4 No 0/4	Yes 0/4 No 4/4
Your result (% sperm bound to slide)	81	78	87	42
Does this indicate normal maturity/physiological function?	Yes	No	Yes	No
Comment	Acceptable	Acceptable	Acceptable	Acceptable
Overall statistic				
Mean	80.3	74.8	79.7	39.4
SD	6.9	12.4	8.2	16.1
Range	[71.3-88]	[57.1-86]	[68.8-87]	[25-61]
Your bias	0.9%	4.3%	9.2%	6.6%
Points to note				


HB425

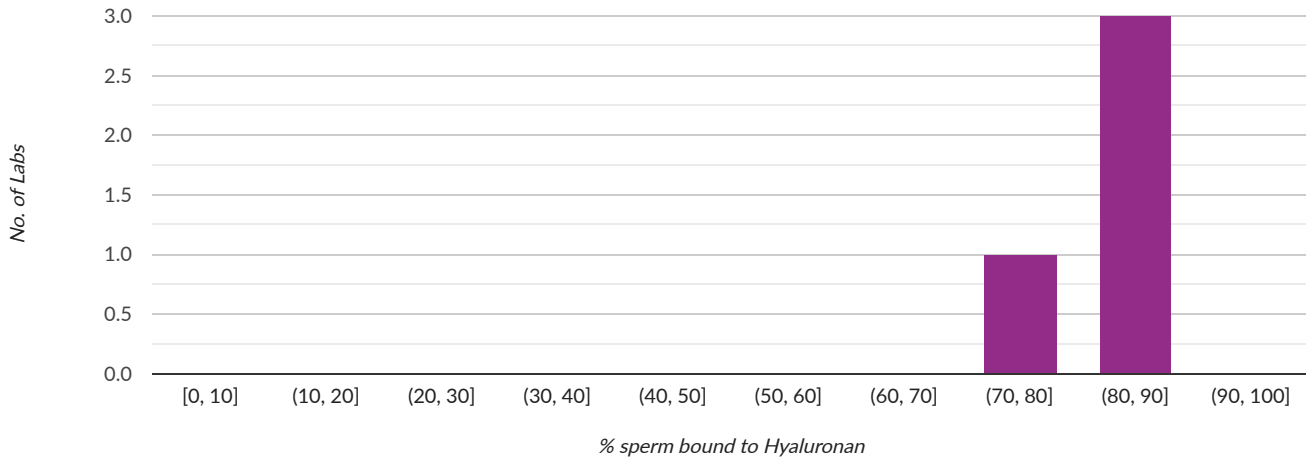


HB426

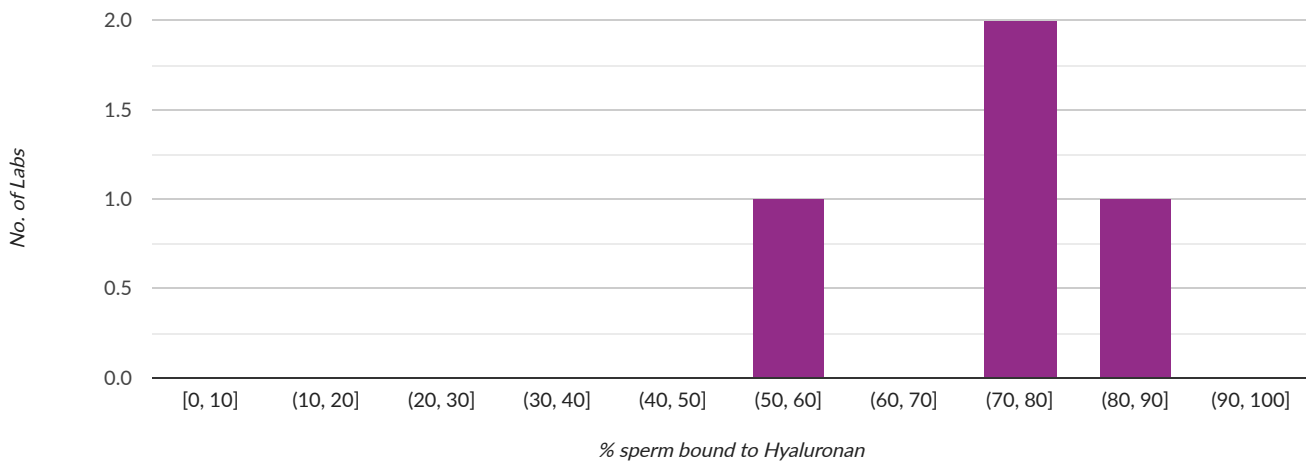


HB427

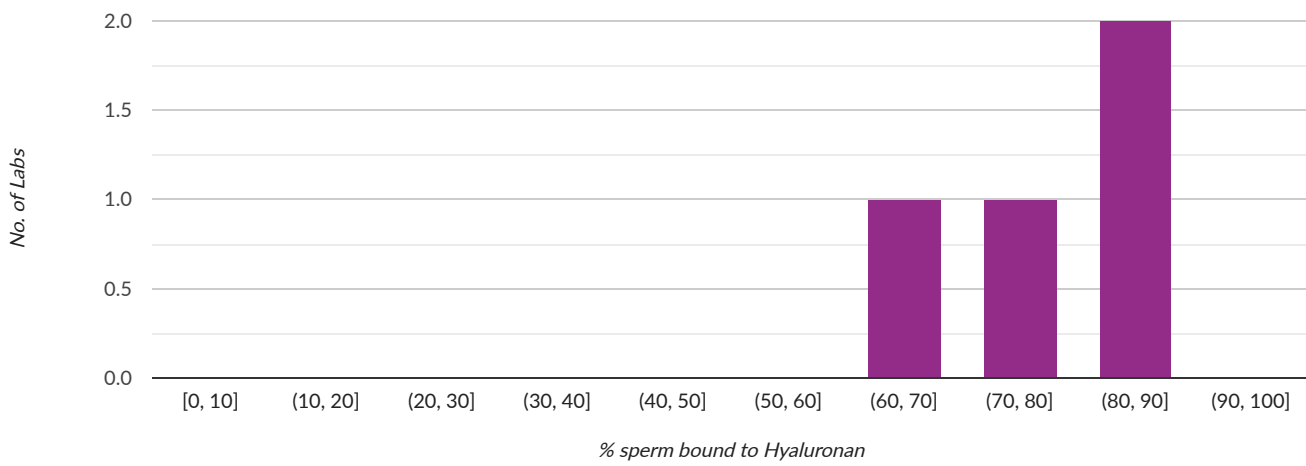

HB428

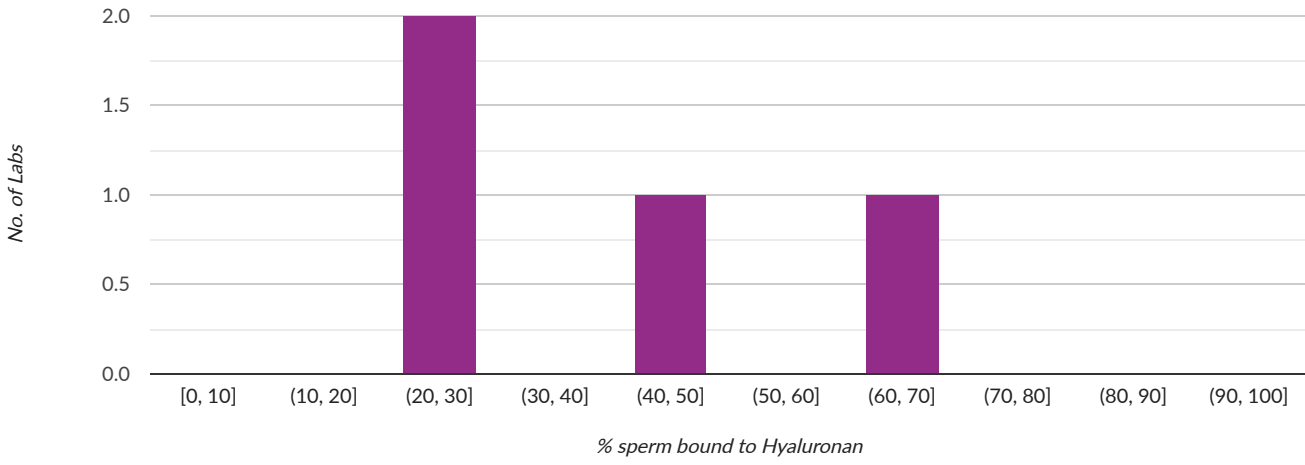

Bias

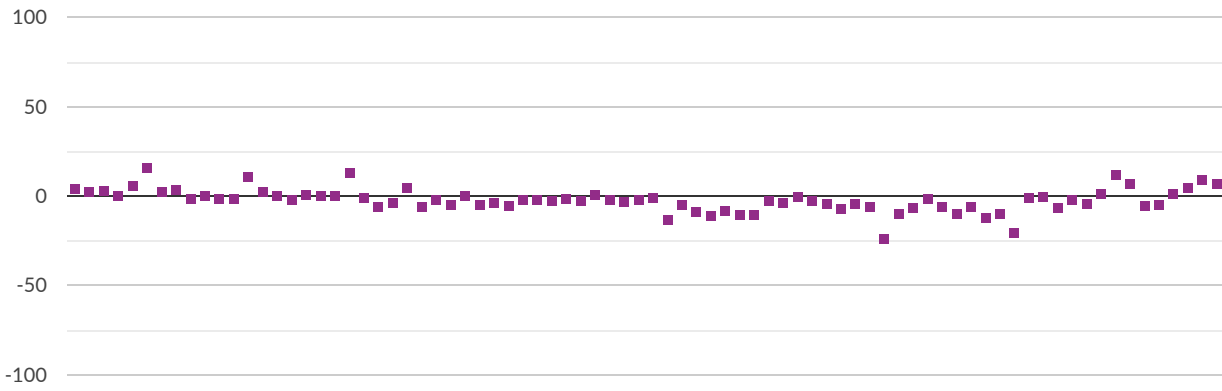

You can alter the date range of results by grabbing and sliding the ends of this section.

