

Scheme: Sperm-hyaluronan assay

Distribution: Q4/4 - 2023/2024

Lab name: LabMagister

Lab number: 971

Reviewed by:


Date:

Action taken:


I Dr Mikus Endre on behalf of LabMagister have read and agreed to the terms and conditions outlined by EQASRM.

Sample code	HB429	HB430	HB431	HB432
Description	Semen sample I	Semen sample II	Semen sample III	Semen sample IV
Number of returns	5	5	5	5
Responses for normal maturity/physiological function	Yes 4/4 No 0/4	Yes 4/4 No 0/4	Yes 4/4 No 0/4	Yes 4/4 No 0/4
Your result (% sperm bound to slide)	89	82	92	84
Does this indicate normal maturity/physiological function?	Yes	Yes	Yes	Yes
Comment	Acceptable	Acceptable	Acceptable	Acceptable
Overall statistic				
Mean	89	80	87.8	80.5
SD	1.4	5.1	3.3	4.4
Range	[87-90]	[73-85]	[84-92]	[75-84]
Your bias	0.0%	2.5%	4.8%	4.3%
Points to note				


HB429

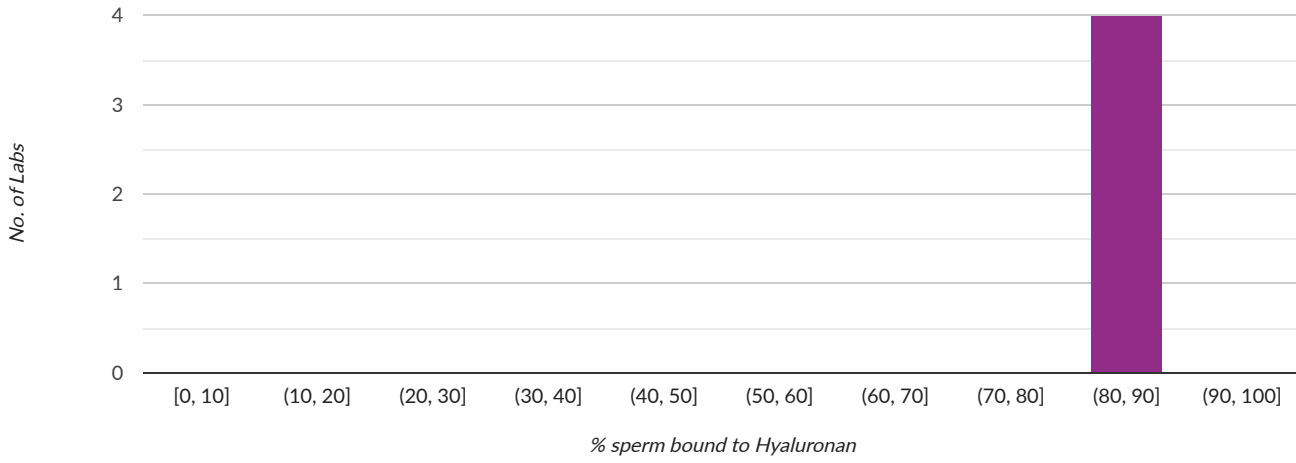


HB430

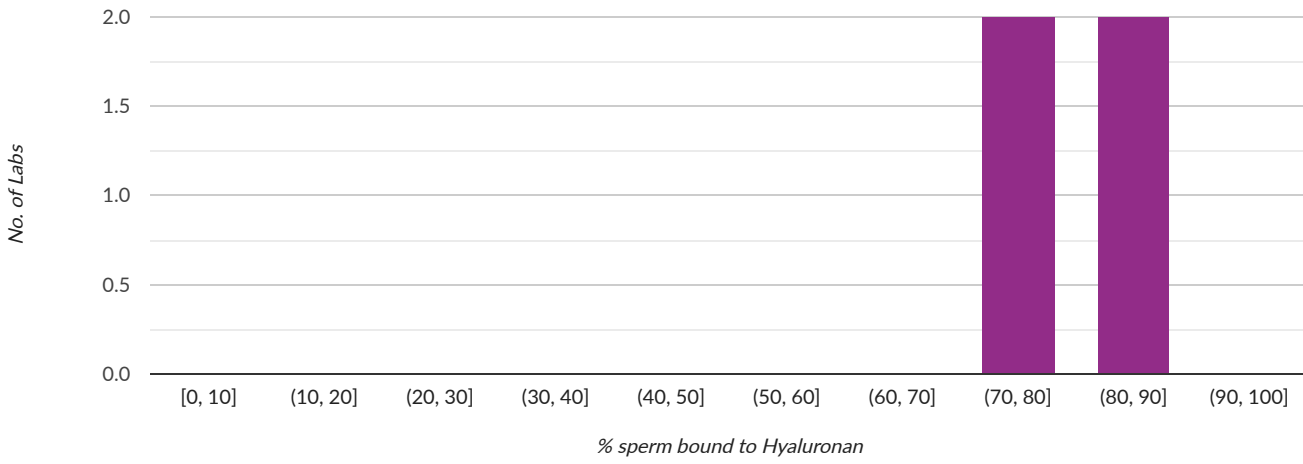


HB431

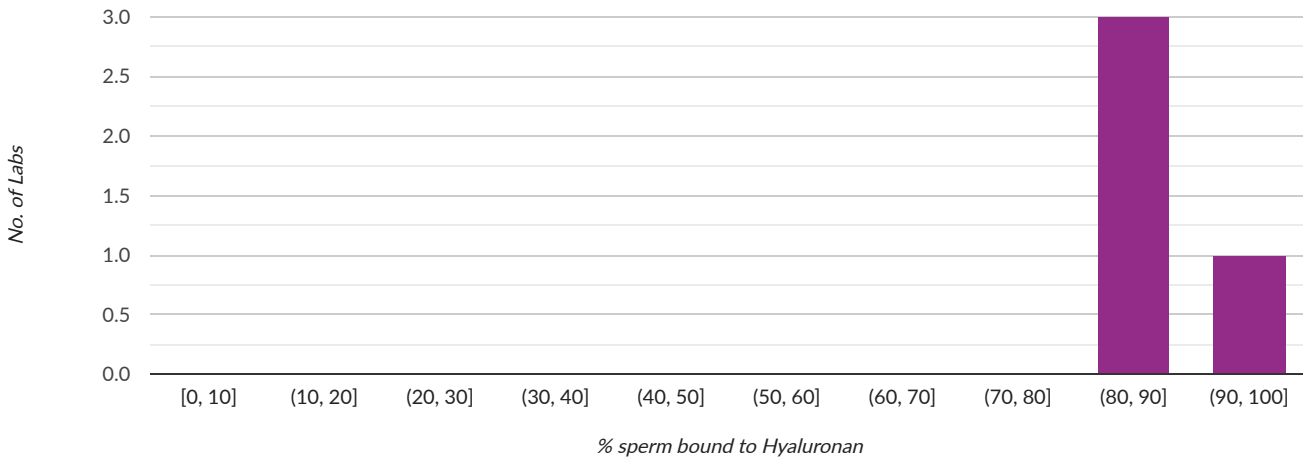

HB432

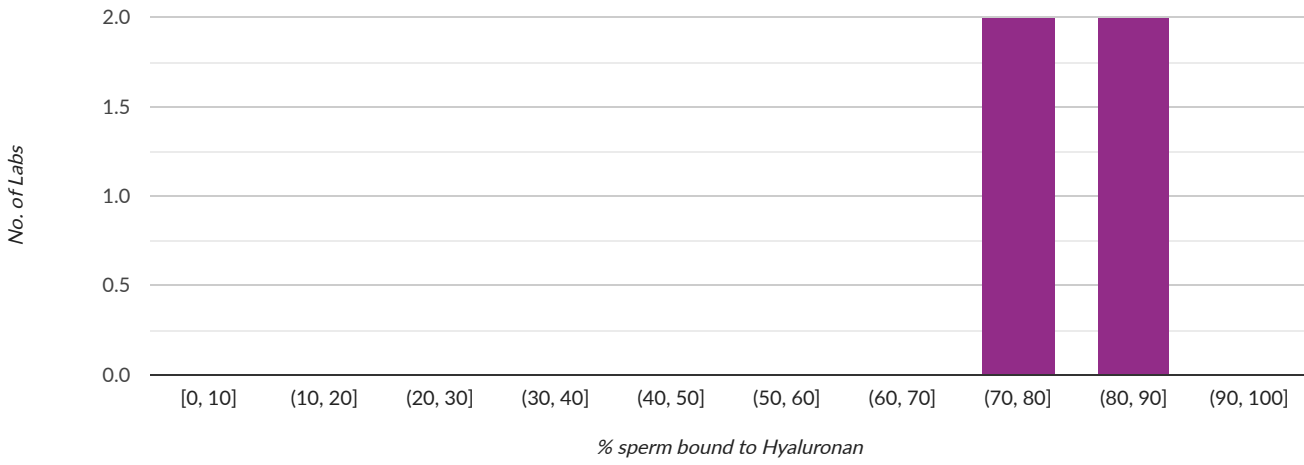

Bias

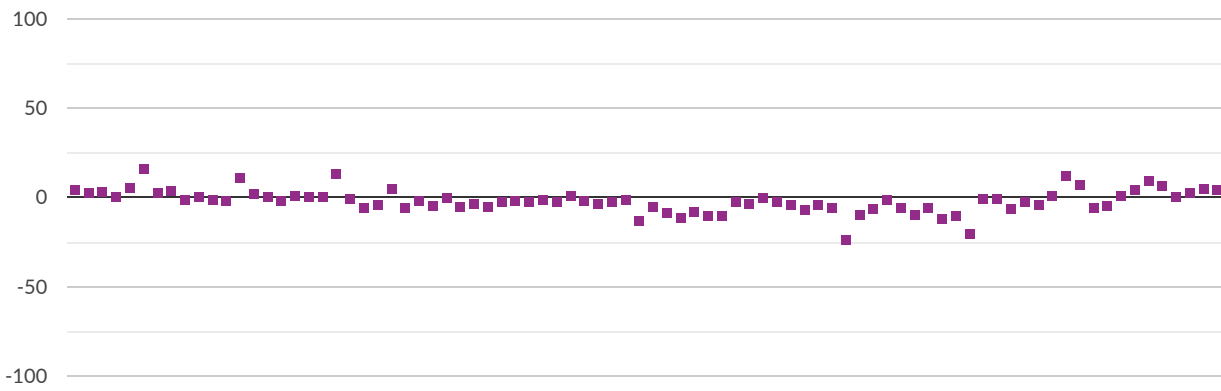

You can alter the date range of results by grabbing and sliding the ends of this section.

